

FIG. 1

Prediction Error for *In Vivo* Measurement of Blood Glucose Concentration

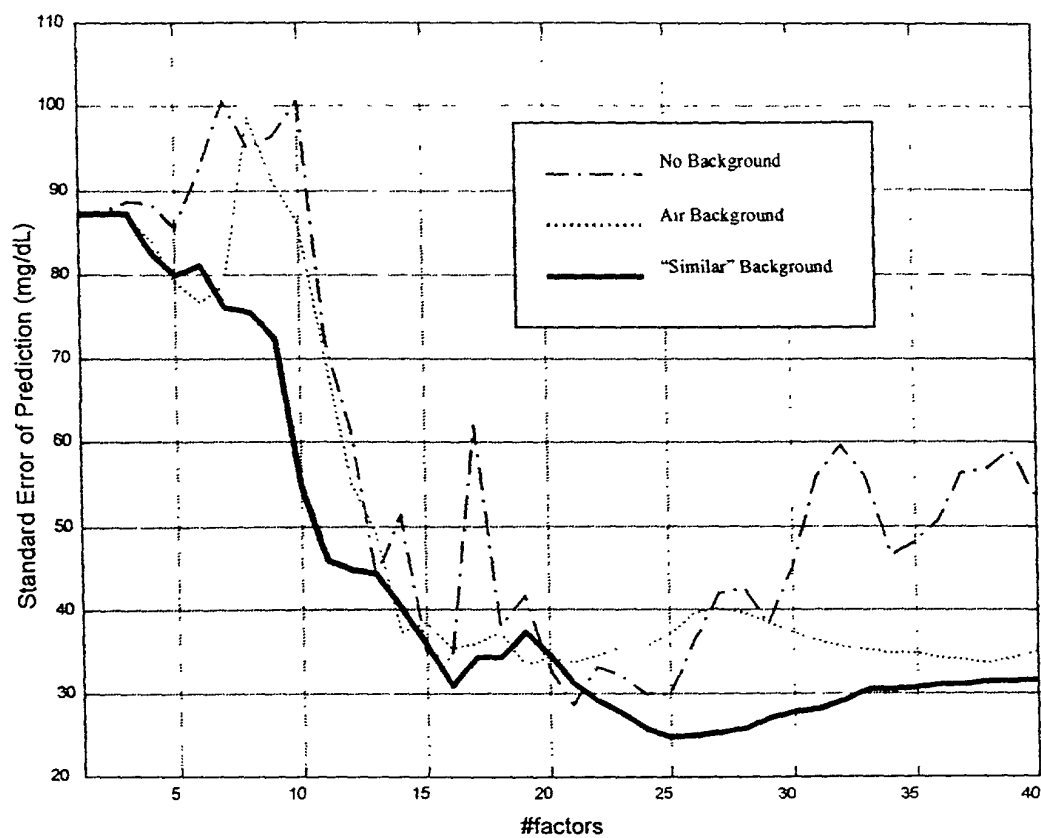


FIG. 2

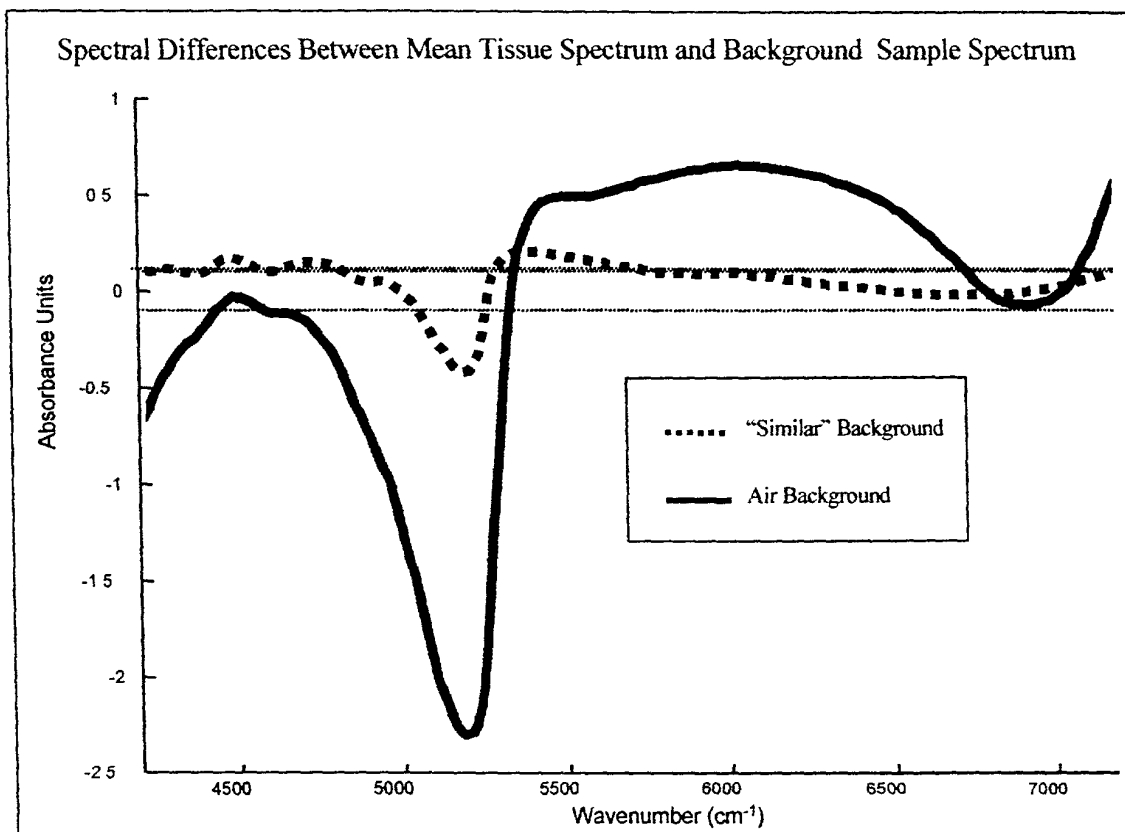


FIG. 3

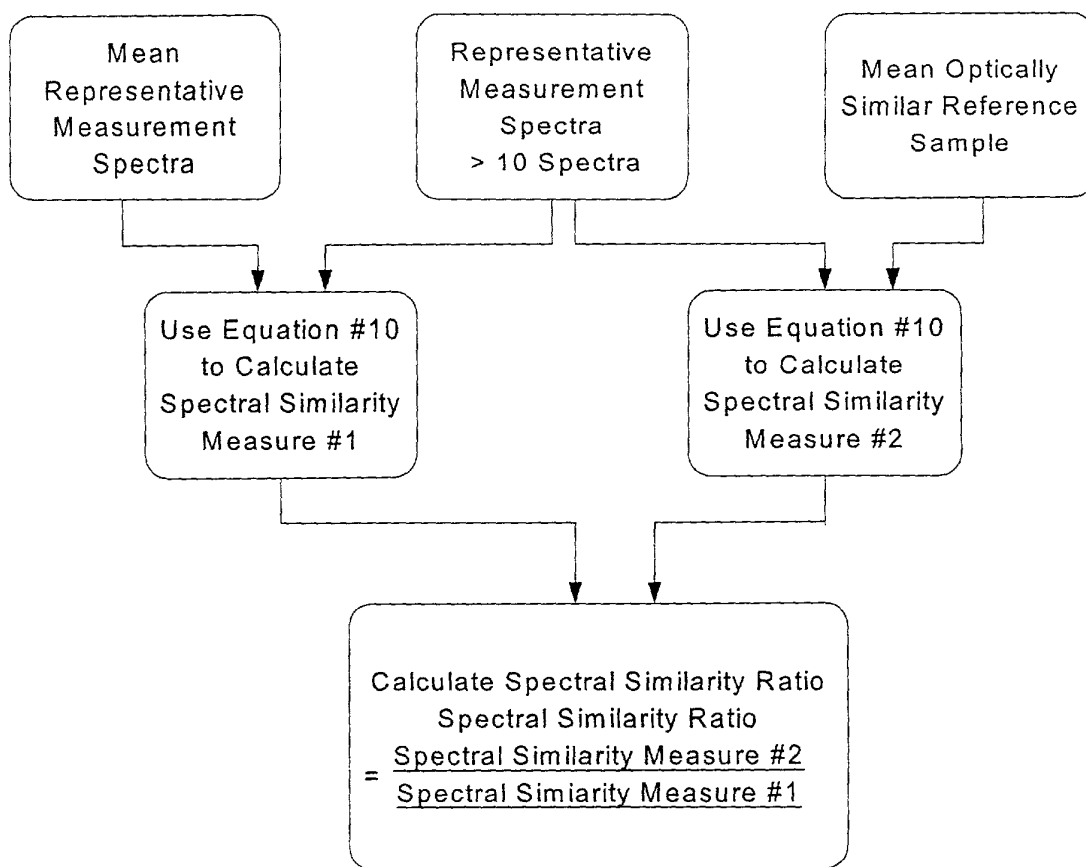


FIG. 4

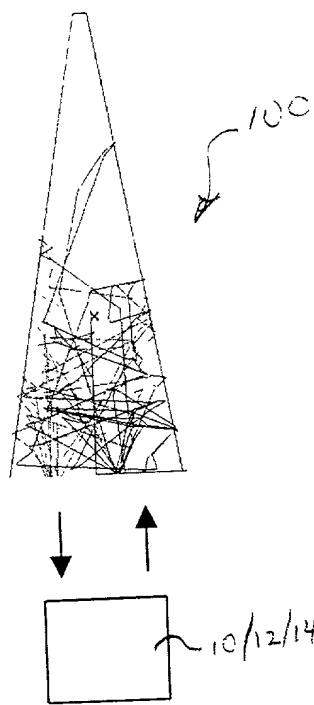


FIG. 5

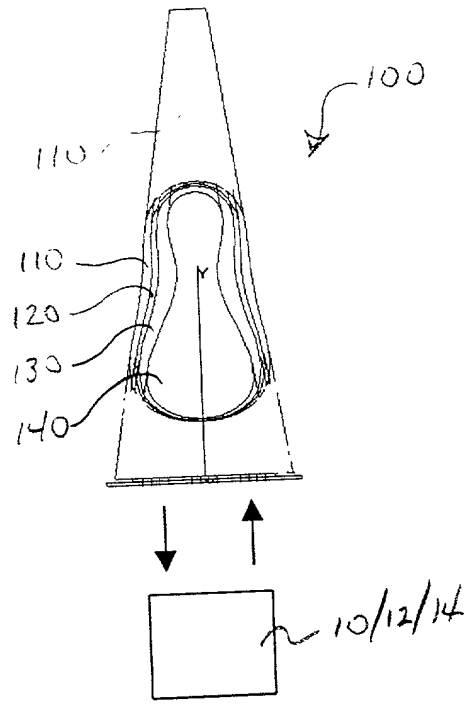


FIG. 6

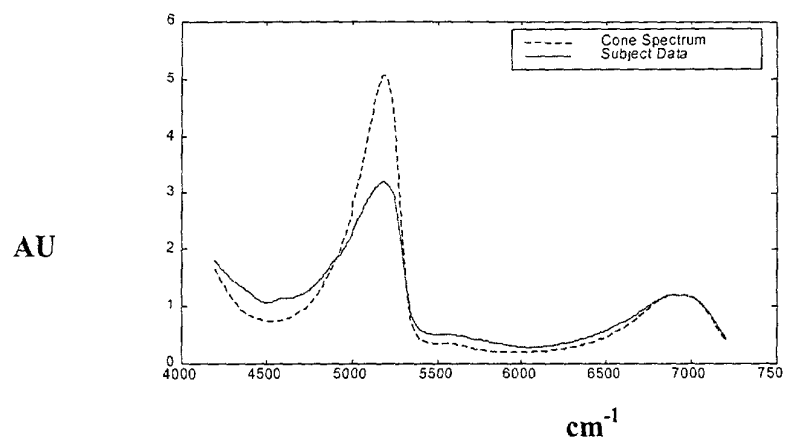


FIG 7

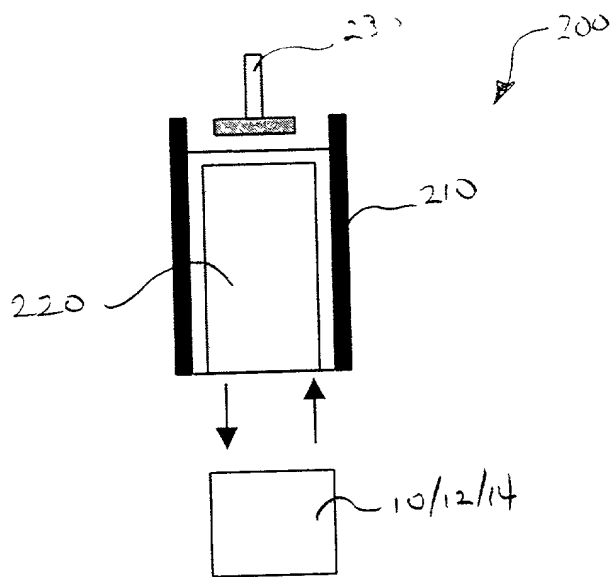


FIG. 8

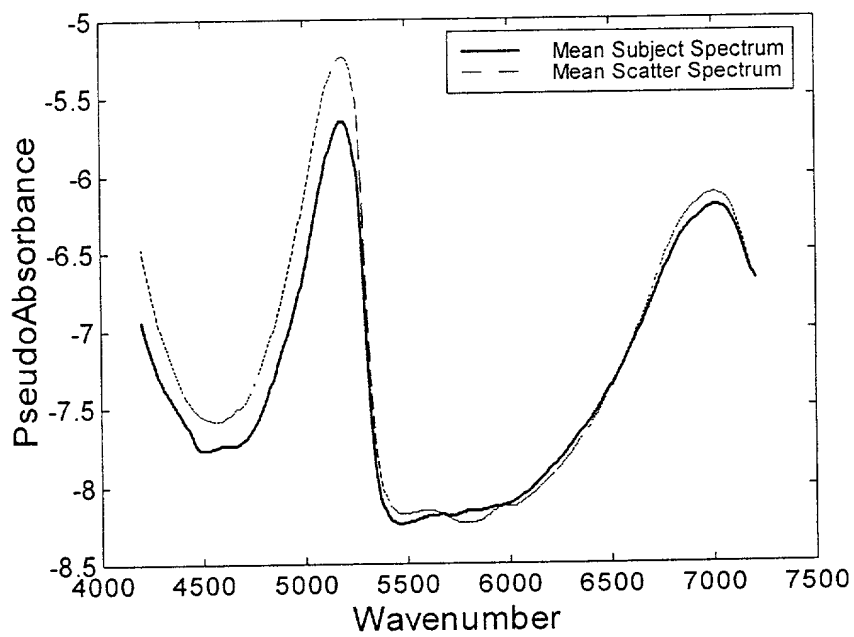


FIG. 9

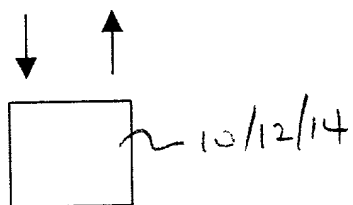
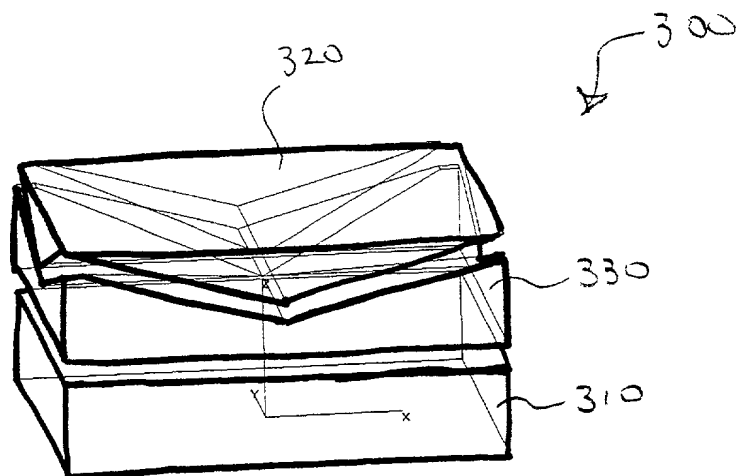


FIG. 10A

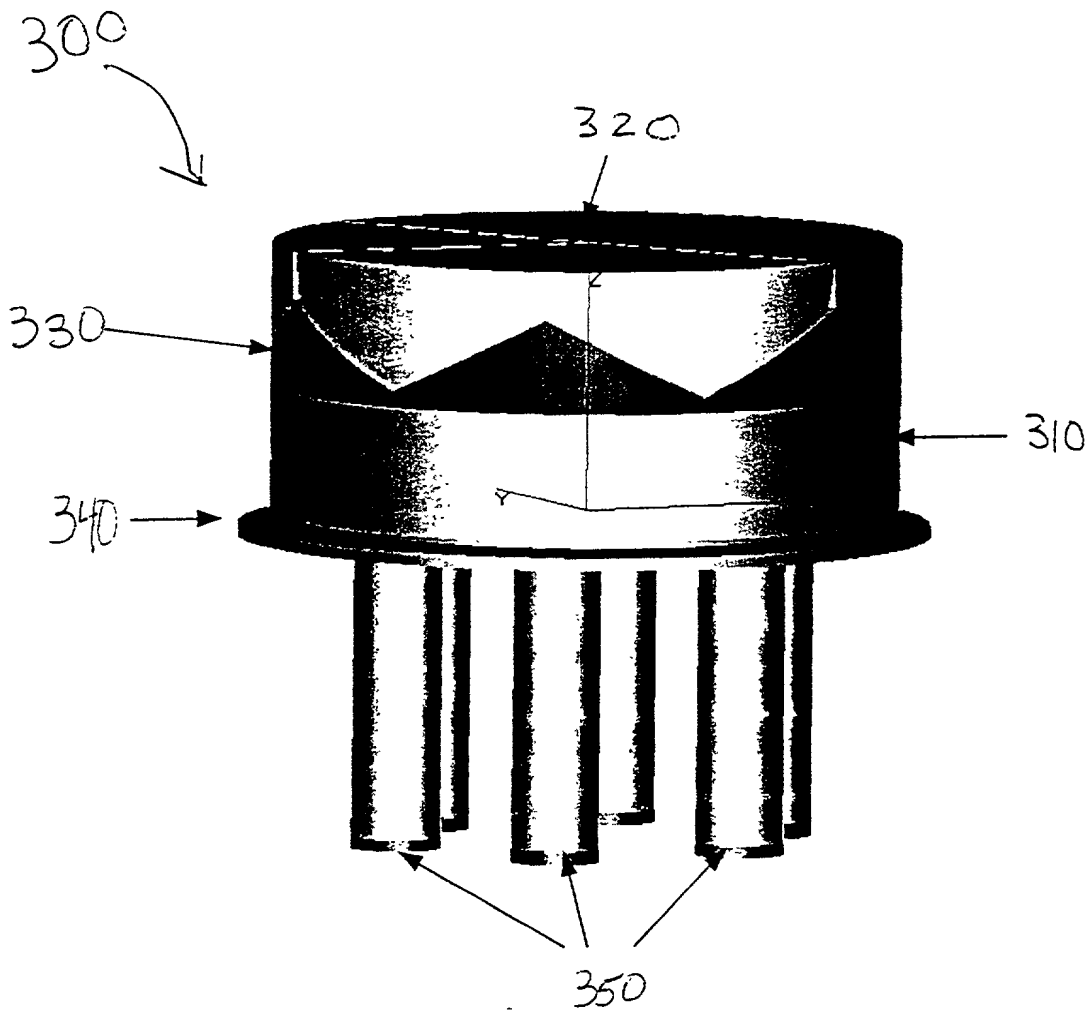


Fig. 10B

AU

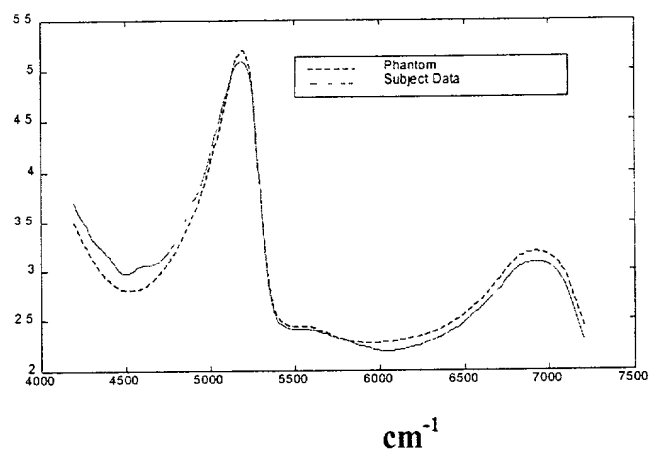


FIG. 11

FIG. 11

FIG. 12

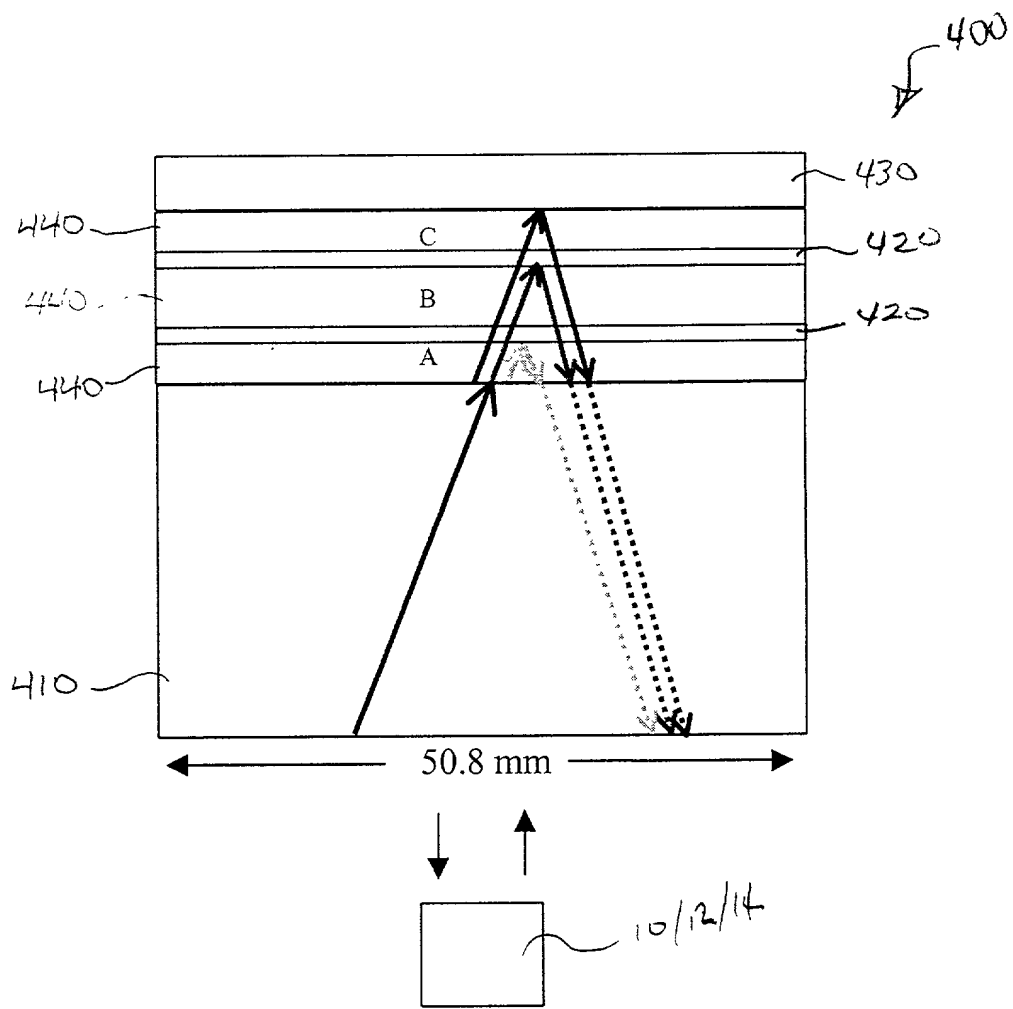


FIG. 12

AU

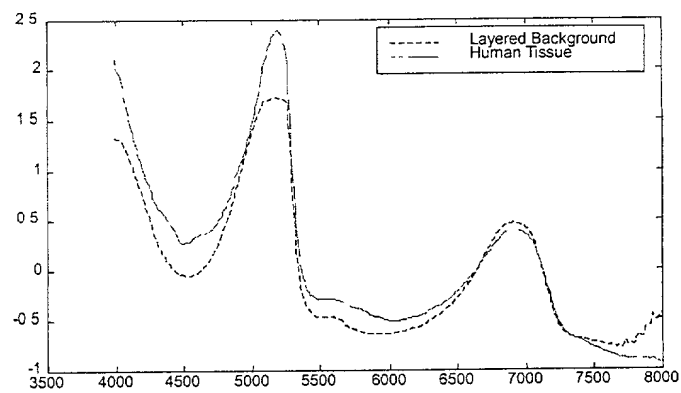


FIG. 13

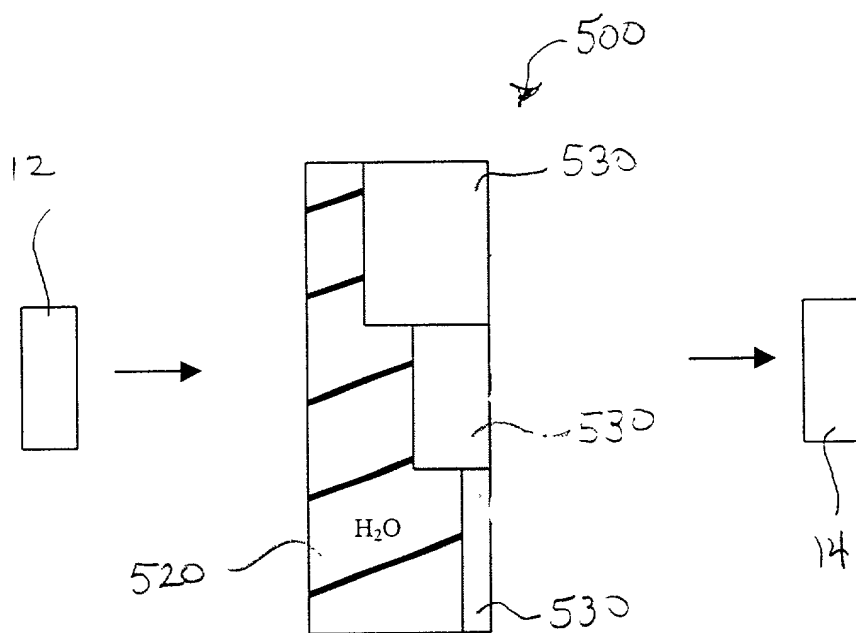


FIG. 14

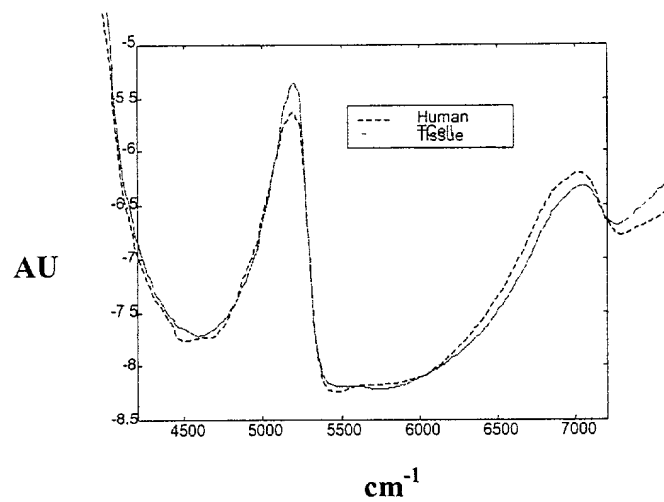


FIG. 15

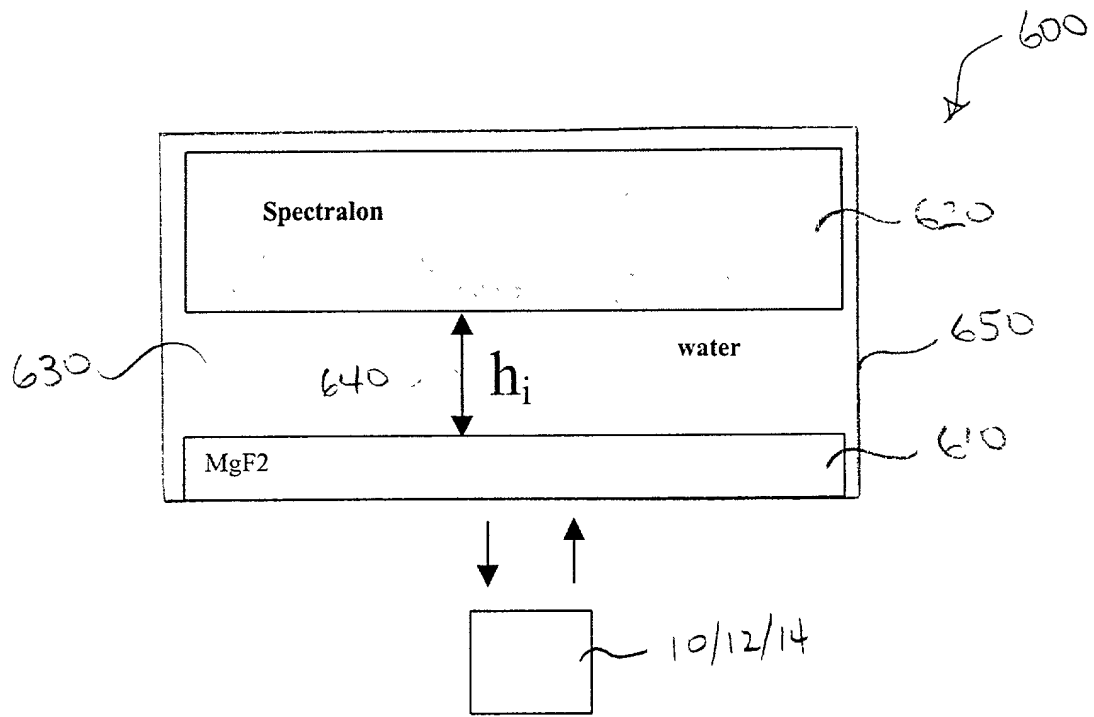


FIG. 16

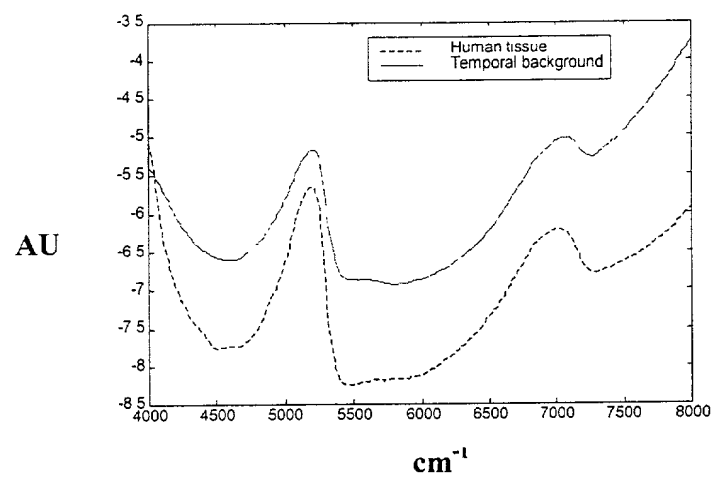


FIG. 17

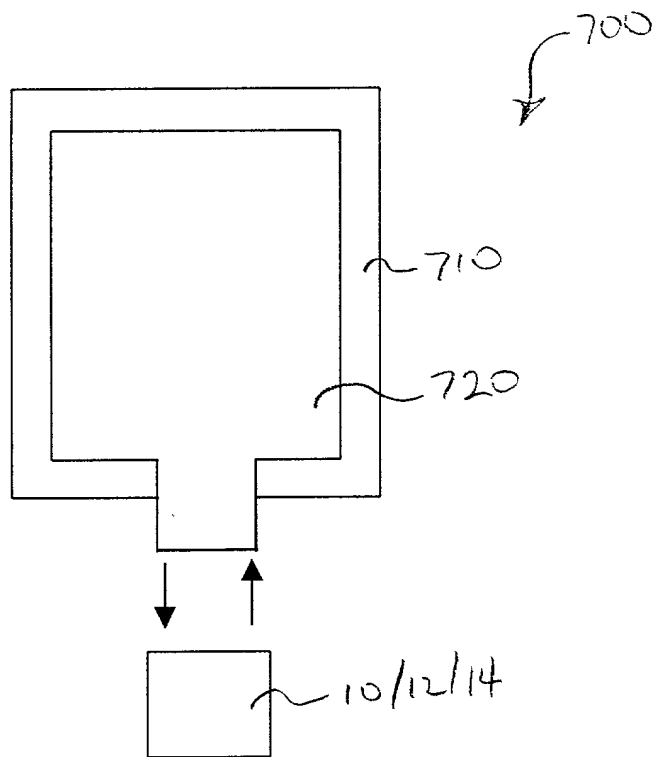


FIG. 18

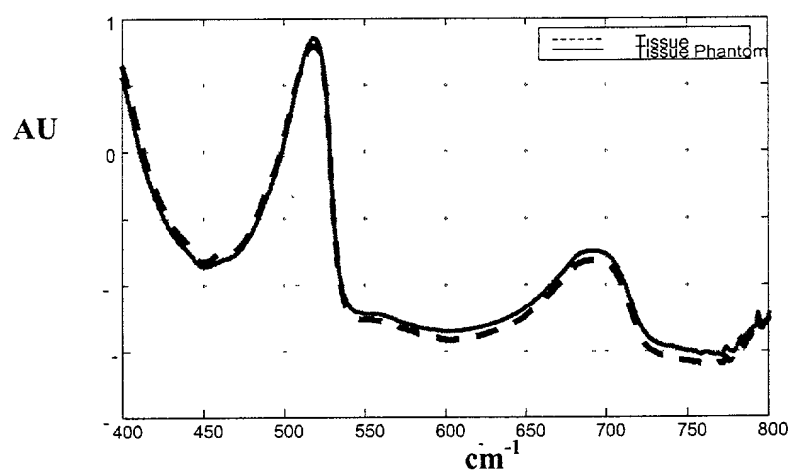


FIG. 19


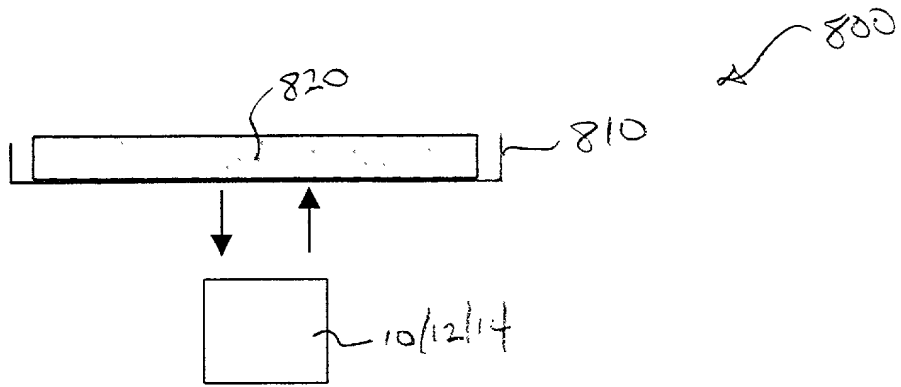


FIG. 20

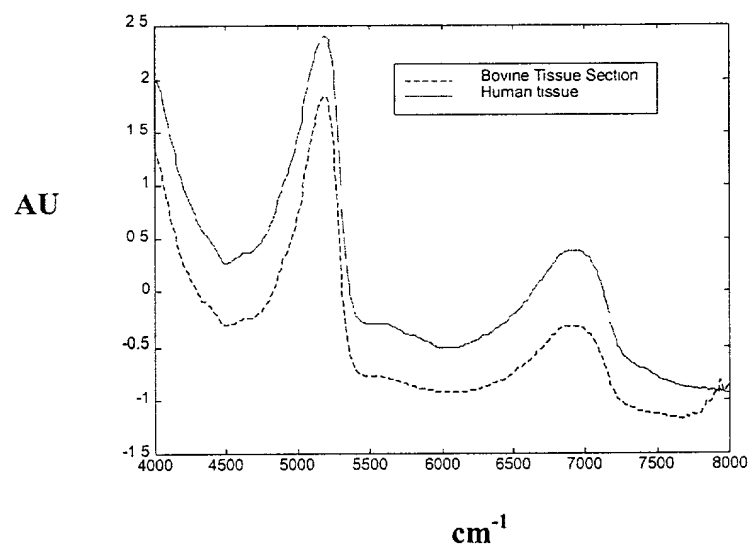

cm⁻¹
FIG. 21